

# Eliminate Daily Maintenance with the D-100 System


Assuming an annual throughput of 60,000 A1c tests, lab operators would need to perform system cleaning on the D-100 System once every 30,000 tests, or twice a year. The cleaning procedure takes only 15 minutes and is fully automated — no operator hands-on time is required. Other HPLC and immunoassay methods require routine daily maintenance.


## Which maintenance routine would you prefer?

**D-100 System — SMART HPLC**



**Immunoassay and other HPLC systems**

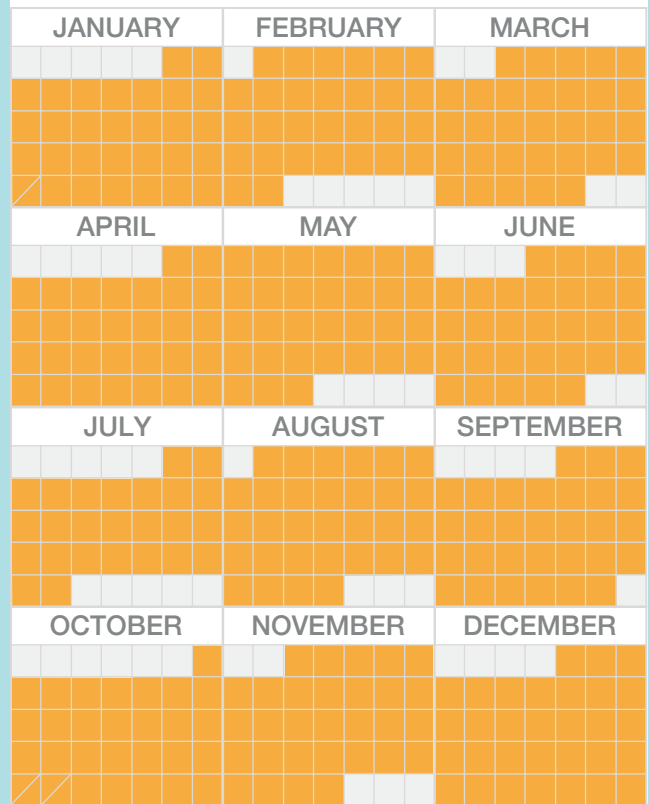

 Scheduled Hands-on Maintenance